

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARWF-0369
Location:	ROBBINSVILLE TWP. P.D.	
Calibration File No.:	01497	Calib. Date: 12/13/2016
Certification File No.:	01498	Calib. No.: 00032
Linearity File No.:	01499	Cert. Date: 12/13/2016
Solution File No.:	01504	Cert. No.: 00024
Sequential File No.:	01504	Lin. Date: 12/13/2016
		Lin. No.: 00024
		Soln. Date: 01/12/2017
		Soln. No.: 00241
		File Date: 01/12/2017

Calibrating Unit:	WET	Model No.: CU-34	Serial No.: DDWJ S3-0329
Control Solution %:	0.100%		Expires: 09/07/2018
Solution Control Lot:	201609A		Bottle No.: 0464

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	18:02S		
Control 1 EC	0.101%	18:02S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	18:02S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:03S		
Control 2 EC	0.100%	18:04S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	18:04S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:05S		
Control 3 EC	0.101%	18:05S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	18:05S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:06S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: HAUGH

First Name: WAYNE

MI: H

Signature:

Badge No.: 37

Date: 01/12/2017

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARWF-0369
Location:	ROBBINSVILLE TWP. P.D.		
Calibration File No.:	01497	Calib. Date:	12/13/2016
Certification File No.:	01498	Cert. Date:	12/13/2016
Linearity File No.:	01499	Lin. Date:	12/13/2016
Solution File No.:	01515	Soln. Date:	03/02/2017
Sequential File No.:	01515	File Date:	03/02/2017
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDWJ S3-0323
Solution Control Lot:	201609A	Expires:	09/07/2018
		Bottle No.:	0463

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:59S		
Control 1 EC	0.100%	07:59S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	07:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:00S		
Control 2 EC	0.100%	08:01S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	08:01S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:01S		
Control 3 EC	0.100%	08:02S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	08:02S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:03S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: MOORE

First Name: JAMES

MI: R

Signature: _____

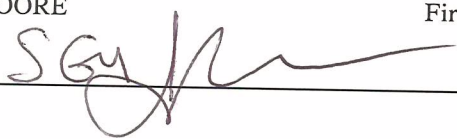

Badge No.: 312

Date: 03/02/2017